


**Series:** 1200VA Universal  
**Model Number:** PM-09239-00

Plitron Manufacturing Inc. Medical PIUs (Power Isolation Units) provide the ultimate in AC power conditioning and low leakage current utilizing unique toroidal transformer technologies from PLITRON with the best surge suppression.



CSA/UL/IEC  
60601-1

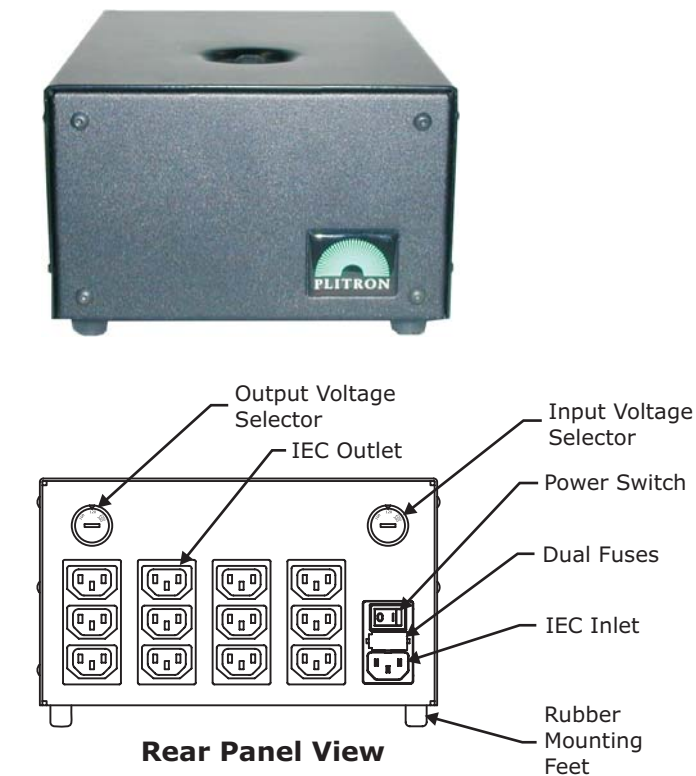

Medical PIUs use series-mode surge removal filters to absorb dangerous voltage surges and safely dissipate them without using failure-prone MOVs (metal oxide varistors). Also, unlike MOV-based protection, voltage surges are not shunted to ground.

### Technical Specs:

**Input Voltage and Frequency:**

Rated 100-120-230/240VAC selectable, 50/60Hz.  
Range +/- 10%V, 47-63Hz

**Input Current:** 10.0A@100V, 10.0A@120V, 5.2A@230V, 5.0A@240V.

**Input (inlet) connector Rear panel:** IEC Inlet

**Leakage Current:** 70µA (Measured at 110% Rated Voltage)

**Load Regulation:** 3.00%

**Output voltage:** 100-120-230/240VAC, selectable

**Output Current:** 9.0A@100V, 9.0A@120V, 5.2A@230V, 5.0A@240V.

**Output connector:** IEC Outlets

**Surge Suppression:** Surges of up to 6000volts (1.2 X 50µSec industry standard rating), with the clamping voltage onset of 344volts peak.

**Operating Temperature:** 25° C Ambient  
Maximum case temperature 55°C

**Weight:** 54.0lbs (24.5Kg)

**Size:**

**(width x height x length)(inch):** 9.5x5.9x12.5

**(width x height x length)(mm):** 245x153x320

Dimensions are approximate.

### Applicable Regulatory Approvals

CAN/CSA C22.2 No 0-M91	-	General Requirement Canadian Electrical Code, Part II
CAN/CSA C22.2 No 601.1 - M90	-	Medical Electrical Equipment Part I : General Requirement for Safety
CAN/CSA C22.2 No 601.1S1 - 94	-	Supplement No. 1-94 to 601.1 - M90
CSA 601.1 Amendment 2:1998	-	
UL 60601-1	-	Medical Electrical Equipment Part I : General Requirement for Safety
IEC 60601-1:1998	-	Medical Electrical Equipment Part I : General Requirement for Safety, including Amendment 1 (1991) and Amendment 2 (1995)

Medical  
**PIU**

PM-09239-00 Rev. 001	May 1, 2008	1200VA Universal Medical Power Isolation Units
PLITRON Manufacturing Inc.		
#8-601 Magnetic Drive, Toronto, Ontario M3J 3J2 Canada		
www.plitron.com	800-PLITRON (754-8766)	
techinfo@plitron.com	416-667-9914 fax 416-667-8928	

